Infection Control & Hospital Epidemiology (2019), **40**, 106–108
doi:10.1017/ice.2018.298

Concise Communication

Mycobacterium avium pseudo-outbreak associated with an outpatient bronchoscopy clinic: Lessons for reprocessing

Jessica L. Seidelman MD[1,2], Richard J. Wallace, Jr MD[3], Elena Iakhiaeva[3], Ravikiran Vasireddy[3], Barbara A. Brown-Elliott MS[3], Celeste McKnight[4], Luke F. Chen MBBS, MPH, CIC, FRACP[1], Terry Smith MS[3] and Sarah S. Lewis MD, MPH[1,2]

[1]Division of Infectious Diseases, Duke University School of Medicine, Durham, North Carolina, [2]Duke Center for Antimicrobial Stewardship and Infection Prevention, Durham, North Carolina, [3]Department of Microbiology, the University of Texas Health Science Center at Tyler, Tyler, Texas and [4]Duke Clinical Microbiology Laboratory, Duke University Medical Center, Durham, North Carolina (Present affiliation: Merck & Co, Philadelphia, PA [L.F.C].)

Abstract

We identified a pseudo-outbreak of *Mycobacterium avium* in an outpatient bronchoscopy clinic following an increase in clinic procedure volume. We terminated the pseudo-outbreak by increasing the frequency of automated endoscope reprocessors (AER) filter changes from quarterly to monthly. Filter changing schedules should depend on use rather than fixed time intervals.

(Received 9 July 2018; accepted 11 September 2018; electronically published 26 November 2018)

Inadequate high-level disinfection or sterilization of bronchoscopes can result in contaminated bronchoalveolar lavage (BAL) fluids or transmission of opportunistic pathogens that cause colonization or infection of susceptible patients. Nontuberculous mycobacteria (NTM) are ubiquitous in the environment, prone to form biofilms, and resistant to most disinfectants including chlorine, which make them well suited to cause outbreaks.[1–3] Bronchoscope-related NTM outbreaks have been attributed to contaminated automated endoscope reprocessors (AERs).[2]

We identified an increase in positive *Mycobacterium avium complex* (MAC) BAL samples from an outpatient bronchoscopy suite in the fall of 2015. This report describes our investigation of what proved to be a pseudo-outbreak and the measures taken to mediate it.

Methods

The pseudo-outbreak took place at the Duke Clinic, an outpatient clinic operated by Duke University Hospital, a 957-bed tertiary-care hospital in Durham, North Carolina. Duke is a high-volume lung transplant center, and frequent routine post-transplant surveillance bronchoscopies are performed in this clinic. Prior to the outbreak, in October 2014, 2 endoscopy procedural areas were consolidated into a single area. Following the clinic merge, the monthly average volume of bronchoscopies performed in this single clinic increased from 105 to 143. The reprocessing area of the clinic houses 3 AERs; the water source and number of AERs were constant during the study.

Author for correspondence: Jessica L. Seidelman, 310 Trent Drive, Hanes House Room 181, Durham, NC 27710. E-mail: jessica.seidelman@duke.edu

Cite this article: Seidelman JL, *et al.* (2019). *Mycobacterium avium* pseudo-outbreak associated with an outpatient bronchoscopy clinic: Lessons for reprocessing. *Infection Control & Hospital Epidemiology* 2019, 40, 106–108. doi: 10.1017/ice.2018.298

© 2018 by The Society for Healthcare Epidemiology of America. All rights reserved.

Our epidemiologic investigation included (1) review of mycobacterial culture data, (2) inspection of the bronchoscopy clinical and reprocessing areas, and (3) environmental sampling in the bronchoscope reprocessing area. We determined the percentage of positive MAC BAL isolates from the outpatient bronchoscopy clinic from January 2014 through June 2017 and defined the baseline (January 1, 2014, through June 30, 2015), outbreak (July 1, 2015, through February 28, 2016), and post-outbreak (March 1, 2016, through June 30, 2017) periods. The prevalences of MAC-positive cultures were compared between periods using 2-sample *t* tests.

Infection preventionists reviewed reprocessing, endoscope handling and storage, and general cleanliness of the bronchoscopy reprocessing area and clinic environment. As part of the investigation, cultures of biofilm were obtained at the time of routine (quarterly) filter change from tubing distal to the 1-μm, 0.4-μm, and 0.1-μm filters serving one of the AERs. These swab samples were decontaminated with cetylpyridine chloride,[4] and streaked onto Mitchison and Middlebrook 7H11 agar plates.[5] MAC isolates were identified using standard methods, including a commercial molecular probe (AccuProbe, Hologic, Marlborough, MA).

As part of the investigation, a subset of 8 clinical MAC isolates suspected to be related to the pseudo-outbreak, 2 clinical MAC isolates from a different clinical area not suspected to be related to the pseudo-outbreak, and 2 MAC isolates recovered from the AER tubing were submitted for species identification using partial 16S r-RNA gene sequencing and molecular relatedness testing using variable-number tandem repeats (VNTR) typing[6] and pulsed-field gel electrophoresis (PFGE).[7] Subsequently, VNTR was performed on a convenience sample of archived MAC isolates from BAL specimens obtained in the clinic during the baseline (n = 6), outbreak (n = 4), and postoutbreak (n = 4) periods.

https://doi.org/10.1017/ice.2018.298 Published online by Cambridge University Press

Medical records of patients with positive MAC BAL specimens from the outpatient bronchoscopy clinic during the study period were reviewed to determine whether MAC treatment was prescribed. The study was performed as part of standard hospital operating procedures and was exempted from review by the Institutional Review Boards of Duke University and the University of Texas Health Science Center at Tyler.

Results

In total 112 of 2,238 bronchoscopy procedures (5%) during the baseline period yielded positive MAC BAL cultures compared to 173 of 1133 (15%) bronchoscopies during the outbreak period ($P < .0001$). In addition, 34 (40%) unique patients with MAC-positive BAL specimens were started on therapy in the baseline period compared to 23 (13%) in the outbreak period ($P < .0001$). Follow-up of patients for at least 6 months identified no definite development of symptomatic MAC infection following the bronchoscopy procedure among patients with positive BAL cultures during the pseudo-outbreak period.

Multiple bronchoscopes and all 3 AERs were associated with MAC-positive BAL cultures. No major deficiencies in reprocessing, storage, or handling of bronchoscopes were identified. However, we determined that the prevalence of MAC BAL cultures declined abruptly following the routine change of the series of AER rinse water filters and then gradually increased over the next 2 months (Fig. 1). On February 15, 2016, the AER filter exchange frequency was increased to monthly from the AER manufacturer's recommended quarterly exchange schedule. Following this change, the monthly prevalence of positive MAC BAL cultures decreased to below baseline (3%) (Fig. 1).

All 8 isolates from the bronchoscopy clinic and the 2 environmental isolates collected in January 2016 belonged to the same VNTR type no. 51 and were indistinguishable by PFGE, whereas the 2 BAL isolates that were obtained at a different clinical location belonged to a different VNTR type. In the subsequent retrospective analysis of a convenience sample of stored MAC BAL isolates from clinic patients, 5 of 6 (83%) from the baseline period, 3 of 4 (75%) from the outbreak period, and 1 of 4 (25%) from the postoutbreak period belonged to the VNTR type #51. The VNTR type no. 51 isolates were indistinguishable or were closely related by PFGE (Fig. 2).

Discussion

We report a pseudo-outbreak of clonally related *M. avium* isolates that terminated when the AER rinse water-filter change frequency was increased from quarterly to monthly. Prior pseudo-outbreaks from failure of AER water filters have been reported. One study described a pseudo-outbreak of *Burkholderia cepacia* from improper installation of an AER filter.[8] Another study reported a pseudo-outbreak of *M. chelonae* due to contaminated incoming water, water filters, and the AER.[9] We hypothesize that increased procedure volume at our clinic led to increased flow volume through the filters, which resulted in their early failure. We believe this filter failure resulted in contamination of the water

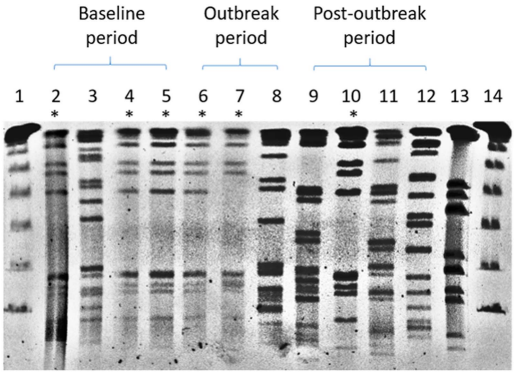


Fig. 2. Pulsed-field gel electrophoresis (PFGE) of AseI restriction enzyme digests of bronchoalveolar lavage (BAL) isolates of Mycobacterium avium from lung transplant patients collected between January 2015 and May 2017. Legend: *denotes VNTR type no. 51. The PFGE pattern for the isolates in lanes 2, 4, 5 (preoutbreak period), 6 (outbreak period), and 10 (postoutbreak period) are indistinguishable; lane 7 (outbreak period) is closely related to the dominant pattern.

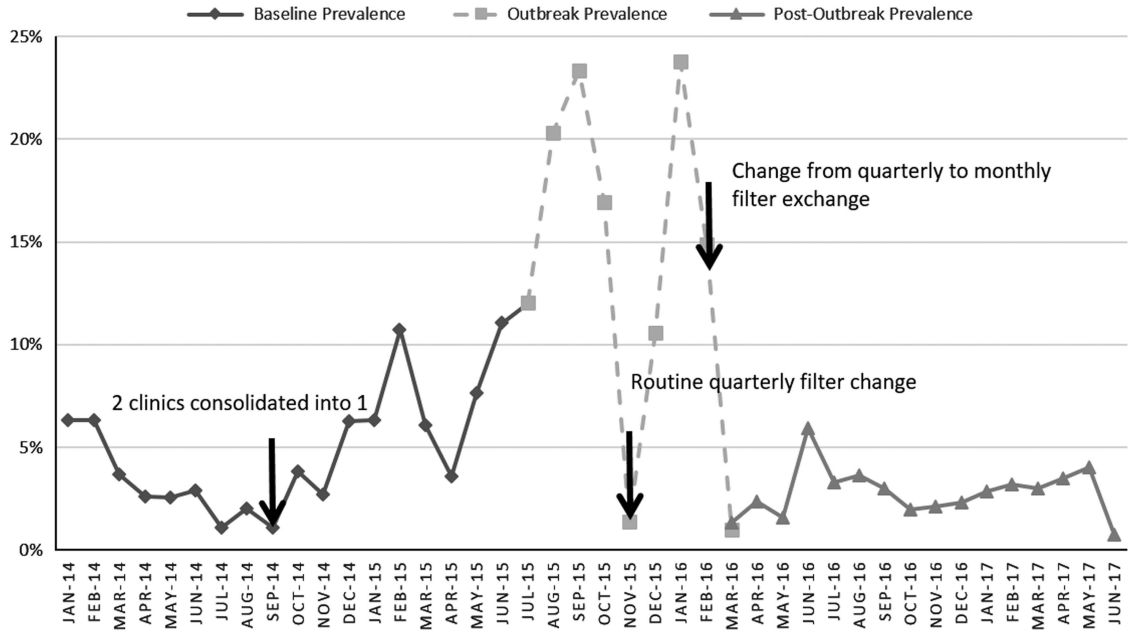


Fig. 1. Monthly prevalence of MAC cultures in the bronchoscopy suite, January 2014 through June 2017.

https://doi.org/10.1017/ice.2018.298 Published online by Cambridge University Press

used to rinse bronchoscopes during reprocessing and resultant contamination of the bronchoscopes themselves.

Bronchoscopy clinics, particularly those with high volume and/or that serve immunocompromised patients, should prospectively review BAL cultures to identify unexpected pathogen trends. Our pseudo-outbreak may have been recognized and terminated sooner had routine surveillance of culture results from the bronchoscopy clinic been performed. The molecular data suggests that the pseudo-outbreak likely began earlier than it was clinically recognized.

Endoscope-related pseudo-outbreaks, including those caused by NTM, continue to occur despite standardized procedures for high-level disinfection of endoscopes. *Mycobacterium avium* and other NTM species, including *M. chimaera* and *M. abscessus*, are known to colonize household and municipal water.[10] Based on our findings, we recommend that routine maintenance schedules for AERs and endoscopes be adjusted based on usage and local water quality rather than a fixed time schedule. Additionally, new technologies, such as disposable endoscopes or endoscopes that can be sterilized, are needed to improve the safety of these devices.

Our study had some limitations. First, differentiating MAC clinical infection from colonization is challenging, particularly in lung transplant patients. Therefore, we were not able to calculate incidence rate of MAC infection in the baseline and outbreak periods. However, the significantly lower proportion of patients who received treatment for MAC disease supports the hypothesis that this was a pseudo-outbreak rather than true outbreak. Second, the filter change frequency from quarterly to monthly was instituted for all 3 filter sizes. We did not experiment with varying the timing of only the terminal filter change, nor did we confirm the exact time at which the filters failed. Finally, molecular sequencing was performed on only a convenient sample of isolates from each study period; therefore, we did not determine the true prevalence of the pseudo-epidemic clone in BALs performed throughout the study period. The molecular data show a decrease in recovery of the *M. avium* pseudo-epidemic clone after the adoption of monthly filter changes. We are unable to determine whether the ongoing recovery of the pseudo-epidemic clone VNTR no. 51 represents ongoing low-level contamination of rinse water or simply indicates that VNTR no. 51 is present in the local municipal water supply and causes colonization or infection in patients when patients are exposed to municipal water via other routes.

In conclusion, we describe a pseudo-outbreak of a single clone of *M. avium* related to failure of the AER rinse water filtration system. Healthcare facilities performing high-volume endoscopy procedures should be aware that AER filters may require replacement based on frequency of use or water quality rather than manufacturers' recommendations based on time in use.

Acknowledgments. None.

Financial support. No financial support was provided relevant to this article.

Conflicts of interest. All authors report no conflicts of interest relevant to this article.

References

1. Kovaleva J, Peters FT, van der Mei HC, Degener JE. Transmission of infection by flexible gastrointestinal endoscopy and bronchoscopy. *Clin Microbiol Rev* 2013;26:231–254.
2. Wallace RJ Jr, Brown BA, Griffith DE. Nosocomial outbreaks/pseudo-outbreaks caused by nontuberculous mycobacteria. *Annu Rev Microbiol* 1998;52:453–490.
3. Collins FM. Bactericidal activity of alkaline glutaraldehyde solution against a number of atypical mycobacterial species. *J Appl Bacteriol* 1986;61:247–251.
4. Falkinham JO 3rd. Nontuberculous mycobacteria from household plumbing of patients with nontuberculous mycobacteria disease. *Emerg Infect Dis* 2011;17:419–424.
5. CLSI. *Laboratory Detection and Identification of Mycobacteria; Approved Guidelines*. Wayne, PA: Clinical and Laboratory Standards Institute; 2008.
6. Iakhiaeva E, Howard ST, Elliott BAB, *et al*. Variable-number tandem-repeat analysis of respiratory and household water biofilm isolates of "*Mycobacterium avium* subsp. *hominissuis*" with establishment of a PCR database. *J Clin Microbiol* 2016;54:891–901.
7. Wallace RJ Jr, Zhang Y, Brown-Elliott BA, *et al*. Repeat positive cultures in *Mycobacterium intracellulare* lung disease after macrolide therapy represent new infections in patients with nodular bronchiectasis. *J Infect Dis* 2002;186:266–273.
8. Rosengarten D, Block C, Hidalgo-Grass C, *et al*. Cluster of pseudoinfections with *Burkholderia cepacia* associated with a contaminated washer-disinfector in a bronchoscopy unit. *Infect Control Hosp Epidemiol* 2010;31:769–771.
9. Chroneou A, Zimmerman SK, Cook S, *et al*. Molecular typing of *Mycobacterium chelonae* isolates from a pseudo-outbreak involving an automated bronchoscope washer. *Infect Control Hosp Epidemiol* 2008;29:1088–1090.
10. Wallace RJ, Iakhiaeva E, Williams MD, *et al*. Absence of *Mycobacterium intracellulare* and presence of *Mycobacterium chimaera* in household water and biofilm samples of patients in the United States with *Mycobacterium avium* complex respiratory disease. *J Clin Microbiol* 2013;51:1747–1752.

https://doi.org/10.1017/ice.2018.298 Published online by Cambridge University Press